



L020917

Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII	Institution:	N/A
Serial Number:	H47600019	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	1/6/2020 1:50:34 PM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

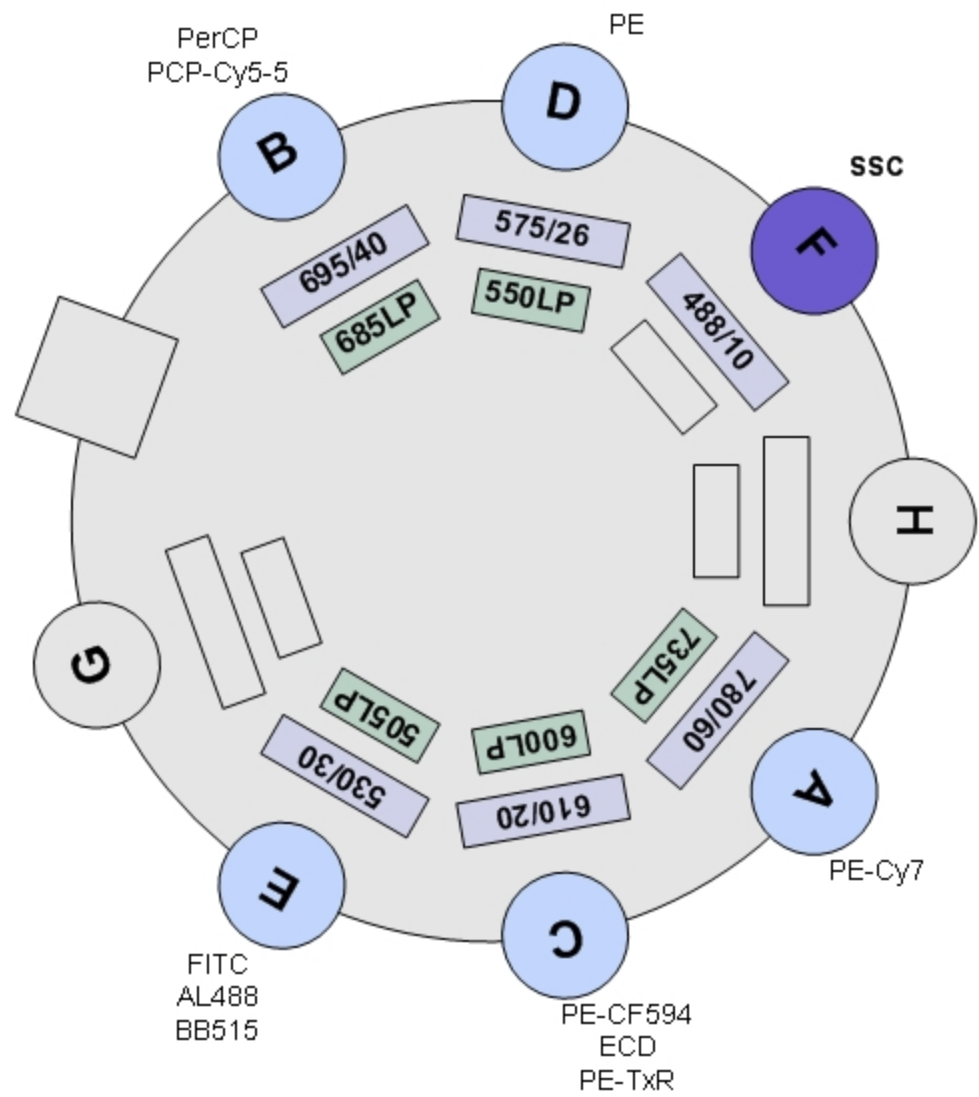


Violet Laser
(405nm)

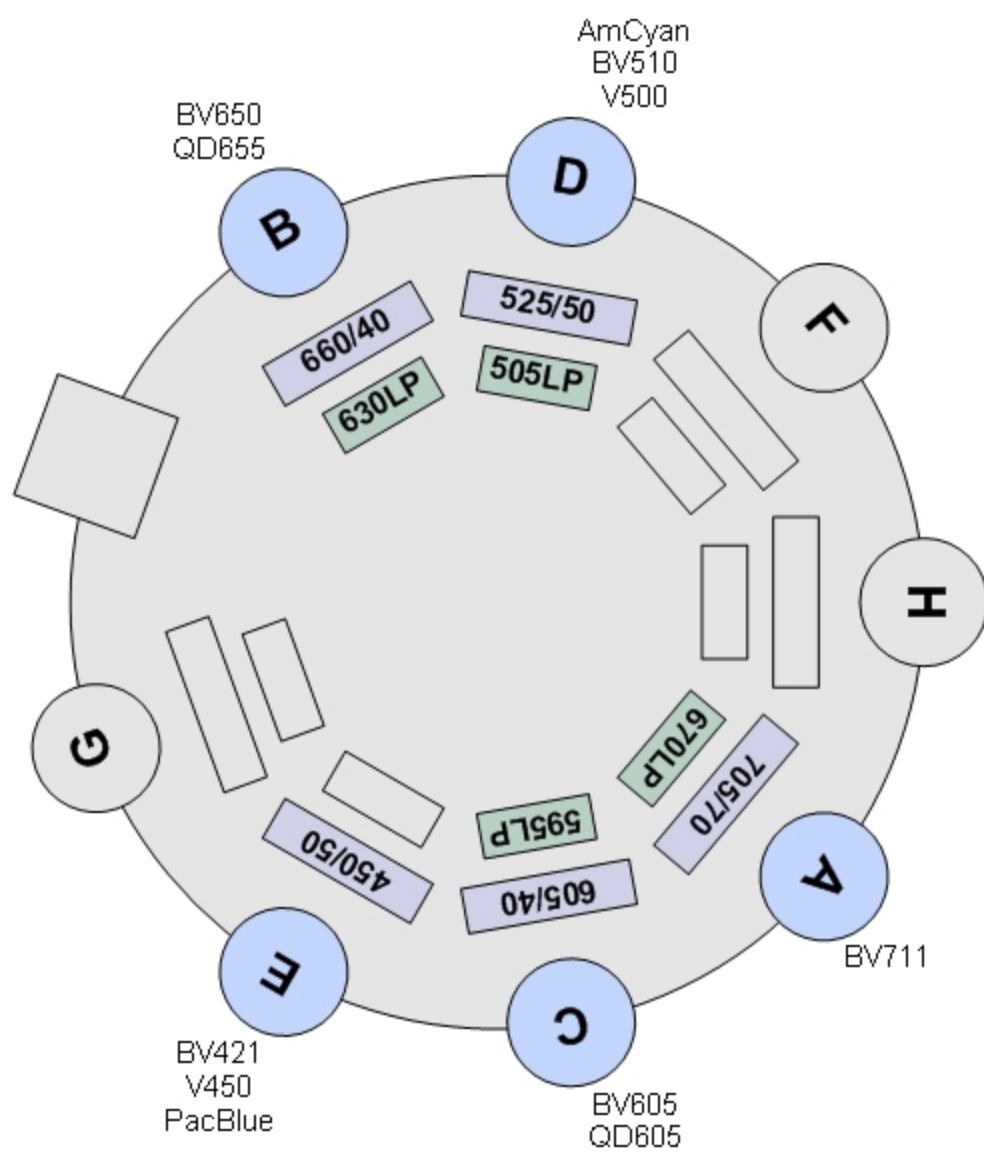

355 UV Laser
(355nm)

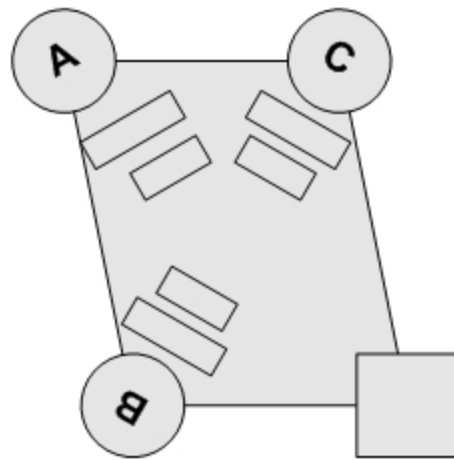

Red Laser
(633nm)

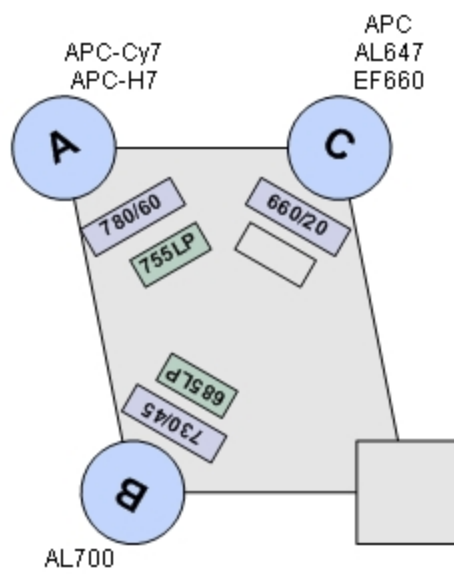

Comments: